

На пути к
долгосрочному
ВОССТАНОВЛЕНИЮ

EDWARDS
MC3 TRICUSPID
кольцо для аннулопластики
Invented by Patrick M. McCarthy, MD



Edwards
LIFESCIENCES

Клинически доказанные предсказуемые результаты

Представляем новое 3D кольцо для аннулопластики от инновационного лидера по клапанной реконструкции.

Учитывая уникальные особенности конструкции, клинически доказанную эффективность и опыт реконструкции у более чем 50 000 пациентов по всему миру, кольцо для аннулопластики Edwards MC3 гарантирует долгосрочное восстановление с предсказуемыми результатами.

Клинически доказанная конструкция


- Реконструкция у более чем 50 000 пациентов по всему миру



Предсказуемые результаты для долгосрочного восстановления


- Многочисленные исследования демонстрируют устойчивую свободу от регургитации трехстворчатого клапана на протяжении длительного времени с использованием кольца Edwards MC3^{1,2,3}

Свобода от повторной регургитации трехстворчатого клапан

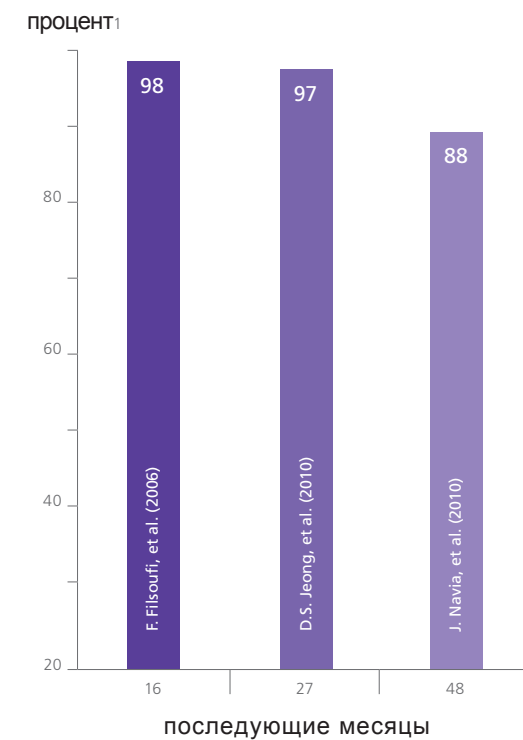


- Устойчивое уменьшение размеров правого предсердия и давления в легочной артерии.^{2,4}

Область правого предсердия⁴

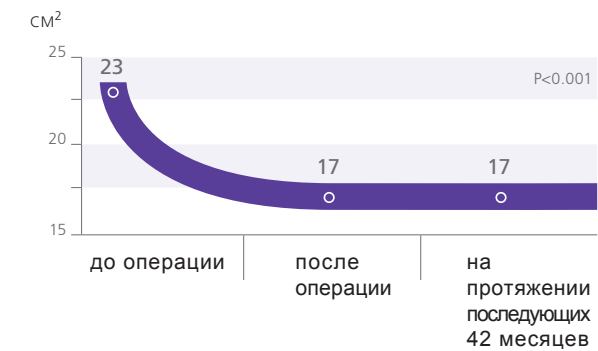


Систолическое давление в легочной артерии²

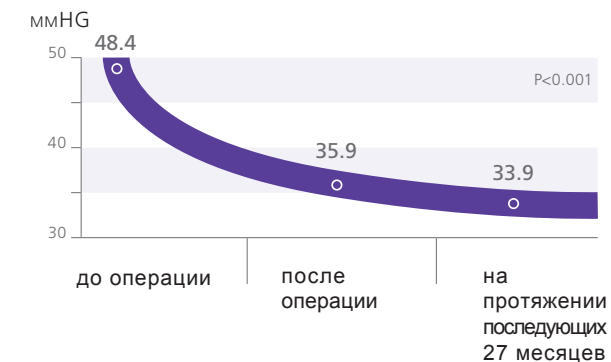

- Свобода от повторной операции в более чем 96 % случаев.^{2,3,5}

Свобода от повторной

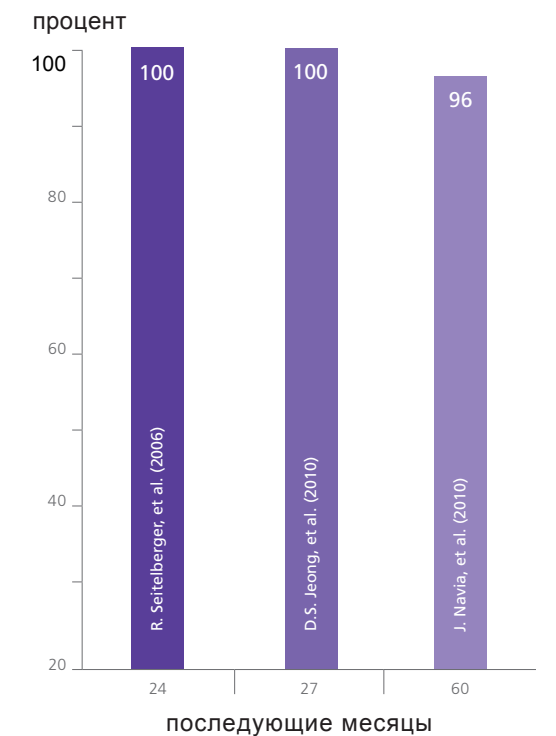

Кольцо для аннулопластики Edwards MC3 Tricuspid

Описание модели	Номер модели
Кольцо для аннулопластики Edwards MC3 Tricuspid (Размеры 26 мм - 36 мм)	4900
Сайзеры	1175
Ручки	1150
Ручка для сайзеров (одноразовая)	1111

Visit Edwards.com or call us at 800.424.3278 for more information.

1. Filsoufi, F., et al. A Three-Dimensional Ring Annuloplasty for the Treatment of Tricuspid Regurgitation. *Ann Thorac Surg* 2006;81:2273-8.
2. Jeong, D.S., MD, PhD., Kim, K.H., MD, PhD. Tricuspid Annuloplasty Using the MC3 Ring for Functional Tricuspid Regurgitation. *Journal of the Japanese Circulation Society*, February 2010;Vol.74.
3. Navia, J., et al. Surgical Management of Secondary Tricuspid Valve Regurgitation. *J Thorac Cardiovasc Surg* 2010:1-10.
4. Fukuda, S., et al. Echocardiographic Follow-up of Tricuspid Annuloplasty with a New Three-Dimensional Ring in Patients with Functional Tricuspid Regurgitation. *J Am Soc Echocardiogr* 2007;20:1236-1242.
5. Seitelberger, R., et al. Surgical Techniques in Patients with Functional Tricuspid Valve Insufficiency: Experience with Two Reconstructive Techniques. *Eur Surg* 2006;38/5:330-337.

For professional use. CAUTION: Federal (United States) law restricts this device to sale by or on the order of a physician. See instructions for use for full prescribing information, including indications, contraindications, warnings, precautions and adverse events.

Dr. Patrick McCarthy receives royalty payments in connection with the Edwards MC3 Ring and is a paid consultant of Edwards Lifesciences.

Edwards is a trademark of Edwards Lifesciences Corporation. Edwards Lifesciences, the stylized E logo and Edwards MC3 are trademarks of Edwards Lifesciences Corporation and are registered in the United States Patent and Trademark Office.

©2010 Edwards Lifesciences Corporation. All rights reserved. AR05512



Edwards Lifesciences